

Ecoflac® Connect S, M, and L

Handling instructions for antiinfective admixture

3 DEVICES, 1 HANDLING PROCESS

Ecoflac® Connect M used here, demonstrates the handling process.

1 Insert Ecoflac® Connect



Remove either one of the tamper-evidence sealing foils of the Ecoflac® plus. Spike transparent end of Ecoflac® Connect into the germ-free port, which does not require disinfection prior to use.

2 Connect the vial



After disinfection of the rubber surface of the vial, insert into the opaque end of the Ecoflac® Connect. A "click" sound confirms the secure connection.

- Ecoflac® Connect **S** fits vials of **13** mm rubber diameter
- Ecoflac® Connect **M** fits vials of **20** mm rubber diameter
- Ecoflac® Connect **L** fits vials of **32** mm rubber diameter

3 Reconstitute



Turn the system upside down. Squeeze and release the walls of Ecoflac® plus in order to inject fluid into the medication vial. Repeat until required volume is present in the vial.

4 Dilute




Turn the system so that the medication vial facing upwards. Apply pressure with two hands on Ecoflac® plus, to dilute the medication into the carrier solution. Label the container per institution SOP.

5 Spike the IV-Set



Remove the second aluminium foil from the Ecoflac® plus. Spike and prime the IV-Set (e. g. Intrafix® SafeSet).

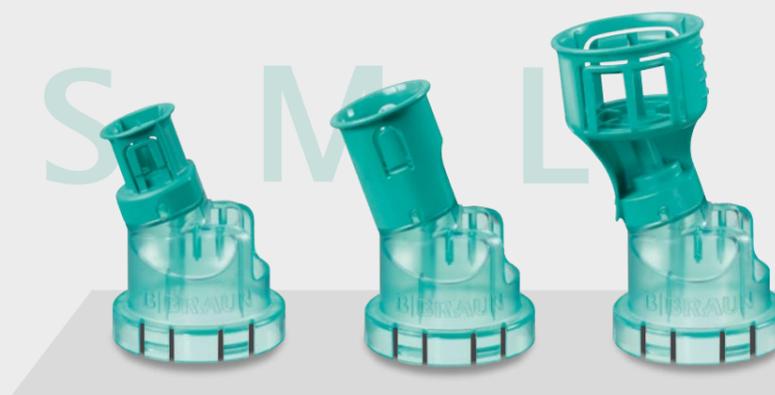

To view a handling video for Ecoflac® Connect or find more information please visit

<https://www.bbraun.com/en/products/b/ecoflac-connect.html>

or scan the adjacent QR-code.